
AFOSR DURIP FA9550-09-1-0496

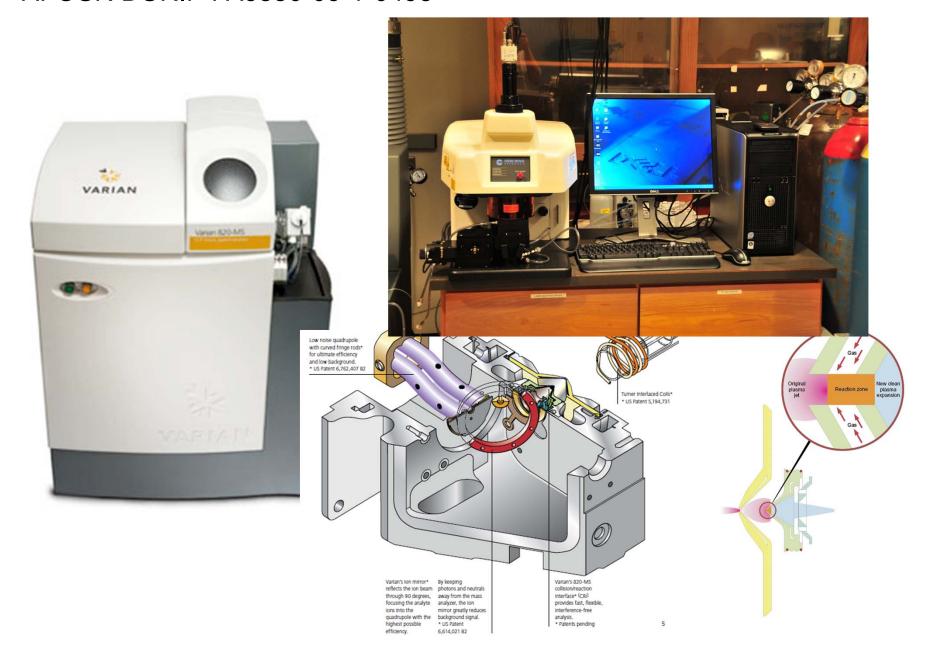

Report Documentation Page

Form Approved OMB No. 0704-0188

Public reporting burden for the collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington VA 22202-4302. Respondents should be aware that notwithstanding any other provision of law, no person shall be subject to a penalty for failing to comply with a collection of information if it does not display a currently valid OMB control number.

1. REPORT DATE 24 DEC 2010	2. REPORT TYPE Final	3. DATES COVERED 15-06-2009 to 14-06-2010	
4. TITLE AND SUBTITLE DURIP - Acquisition of an Induct Spectrometer with Laser Ablation Characterization.	5a. CONTRACT NUMBER FA9550-09-1-0496 5b. GRANT NUMBER		
6. AUTHOR(S)	5c. PROGRAM ELEMENT NUMBER 5d. PROJECT NUMBER		
Guido Verbeck	5e. TASK NUMBER		
7. PERFORMING ORGANIZATION NAME(S) A University of North Texas,1155 U 305250,Denton,TX,76203-5017	5f. WORK UNIT NUMBER 8. PERFORMING ORGANIZATION REPORT NUMBER 6B783		
9. SPONSORING/MONITORING AGENCY NAM AFOSR, 875 North Randolph Str 22203	10. SPONSOR/MONITOR'S ACRONYM(S) 11. SPONSOR/MONITOR'S REPORT NUMBER(S) AFRL-OSR-VA-TR-2011-0221		

12. DISTRIBUTION/AVAILABILITY STATEMENT

Approved for public release; distribution unlimited

13. SUPPLEMENTARY NOTES

14. ABSTRACT

The instrument and projects listed in the brief have been properly installed and executed. The 820 ICP-MS is a universal 90 degree quadrupole mass spectrometer equipped with a collision reaction interface (CRI) front end. The CRI allows low interference which reduces common polyatomic interferences on As, Se, Cr, V and Fe, thus achieving lower detection limits in the plasma, especially for samples with complex matrices. The CRI increases sensitivity and lowers time to acquisition based of the principals that collision dissociation occurs prior to mass selection, eliminating the need for the CID optics in other ICP-MS. Laser Ablation for material characterization is produced from a New Wave (ESI) LS-213 Tempest Laser Ablation System. This is ideal for determining surface composition with ICP-MS. This instrument provided an excellent resource in our multiuser facility and the broad adoption of the ICP-MS technology in industry and academia meant that our students and postdocs can be trained in the most relevant analytical approaches for materials research.


15. SUBJECT TERMS

Softlanding, Preparative Mass Spectrometry, Coatings, Inductively-Coupled Plasma

16. SECURITY CLASSIFICATION OF:			17. LIMITATION OF ABSTRACT	18. NUMBER	19a. NAME OF RESPONSIBLE PERSON
a. REPORT unclassified	b. ABSTRACT unclassified	c. THIS PAGE unclassified	Same as Report (SAR)	OF PAGES 2	







5000000

Legend
200 K
Room Temp (289.92 K)

1000000


Time (s)

Signal RSD vs. Temperature


Isotope	288.92K	250 K	225 K	200 K
51 V	17.49 %	21.31 %	12.76 %	3.18 %
⁶³ Cu	17.92 %	8.05 %	12.42 %	4.32 %


V51 Calibration Curve

V51 Signal vs. Spot Size





Post-Ablation Oil at 200 K

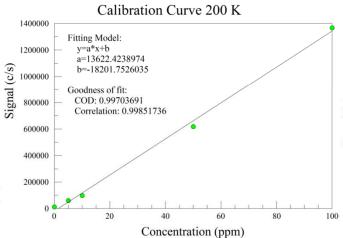


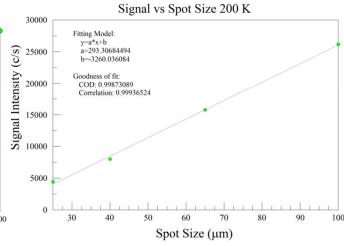


- Collaboration with Dr. Aaron Roberts (UNT Biology Department)
- •Individual Hg202 spectrum for each raster pattern.
- •2D Image created using the Hg202 signal and the X and Y coordinates of the ablated area.

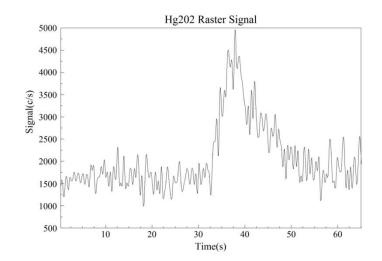


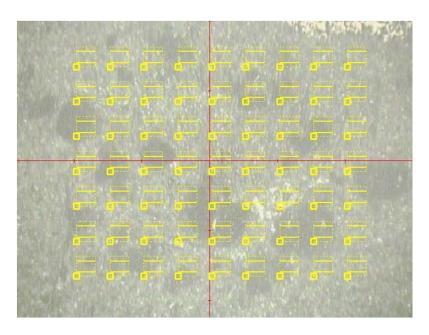

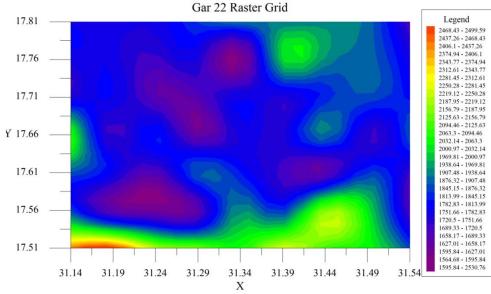

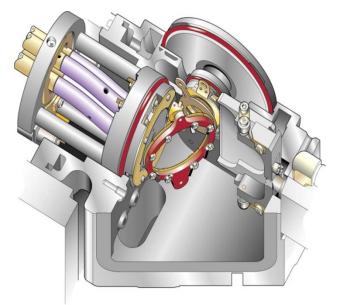

Bruker (Formerly Varian) 820 ICP-MS Ion Optics

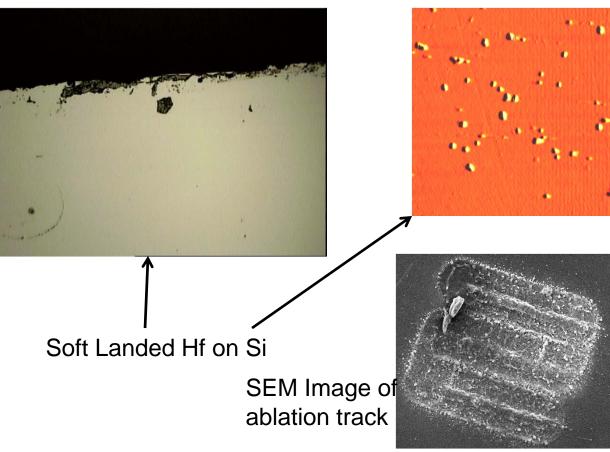

178 Hf Transient Signal on Mica

2000

1500

1000

2000

1000

1000

1000

Time (s)

¹⁷⁸Hf LA-ICP-MS transient signals showing spatially resolved Hf on surface (left) and in defects (right)

